


IVD CE



RSV Ag

Capilia™ RSV Neo

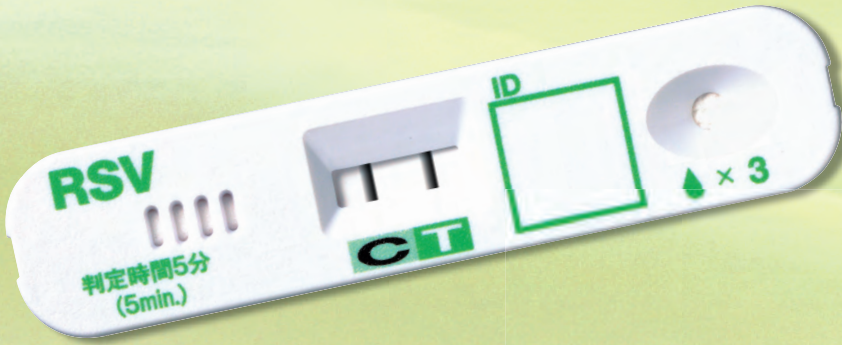


* The sample shows positive result.


- **Rapid test for detecting RS virus antigen**
Permitting accurate results; simple and easy to use
- **Easy to read Black Line**
Adopting the latest nanotechnology, "Platinum-Gold Colloid"
- **Fast test results**
Reading time is 3-5 min.
- **Shared use of extraction buffer in Capilia series**
1 sample can be used for 4 types of tests (Flu, Adeno, hMPV, RSV) at once




more reasonable process, less pain for patients



Collecting specimen



Preparing sample

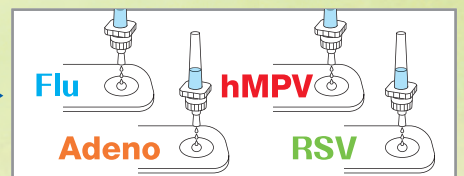

1 sample can be used for up to 4 test plates!

Please follow package insert with each product about shared use of extraction butter.



RS virus Rapid Test Capilia™ RSV Neo

To detect RS virus antigens in nasal swabs or nasal aspirates.




Test Procedure


Method of specimen collection



Sample preparation




Remove the aluminum sealing cap from the extraction buffer tube, while taking care not to spill the liquid.



Soak the swab that collected the specimen in the extraction buffer, and stir well. Then, pinch the tip of the swab firmly with the soft wall of the extraction buffer tube with your fingers and squeeze out the swab. Use this squeezed-out liquid as the sample.


When using a nasal aspirate specimen diluted twofold with physiological saline, add 200 μ L of the specimen to the extraction buffer in the tube, and mix well. Use this mixture as the sample.



Firmly attach the nozzle (with a filter) provided in the kit to the top of the extraction buffer tube.

Sample application

Hold the middle of the tube with the fingers and dispense 3 drops of the sample.

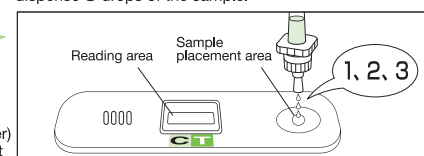

3-5 min

5 min

Reading the result



Reference Data

Clinical data

The result of the clinical performance evaluation in Japan (Comparison with RT-PCR)

Kind of samples	Sensitivity (%)	Specificity (%)	Accuracy (%)	Total number
Nasal swab	86.1 (68/79)	100 (103/103)	94 (171/182)	182
Nasal aspirate	82.1 (69/84)	100 (87/87)	91.2 (156/171)	171

Product Summary

REF CARS0970 (20 Tests)

Kit contents: Test Plate \times 20, Extraction Buffer 0.7 mL \times 20, Nozzle \times 20

REF CARS0971 Test Plate (10 Tests)

Kit content: Test Plate \times 10

Validity: 27 months

Storage: Store at 2-30°C

Reading time: 3-5 minutes